Because we care.

MIDMARK®

Installation

9A283001 IQmark™ Flexible Rotating Mount Holder

KIT COMPONENTS

Part Number	Description	Qty
9A283001	IQmark™ Holder	1
• 050-4906-00	Bracket, Tube Support	1
• 040-0250-88	1/4-20 x 1/2 Hex Bolt	2
• 041-0250-13	1/4-20 Hex Nut	2
• 003-1098-00	Installation Instructions	1

REQUIRED TOOLS

7/16" Wrench

3/8" Socket & Ratchet

INTRODUCTION

Provides a flexible, rotational holder to support the Brentwood IQmark™ device.

CE REPRESENTATIVE

EEC countries should direct all questions, incidents, and complaints to Midmark authorized CE representative: CE

Promotal
22, Rue De St. Dines
53500 Ernie
France
Phone: 33-2-430-517-76
Fax: 33-2-430-569-10

INSTALLATION

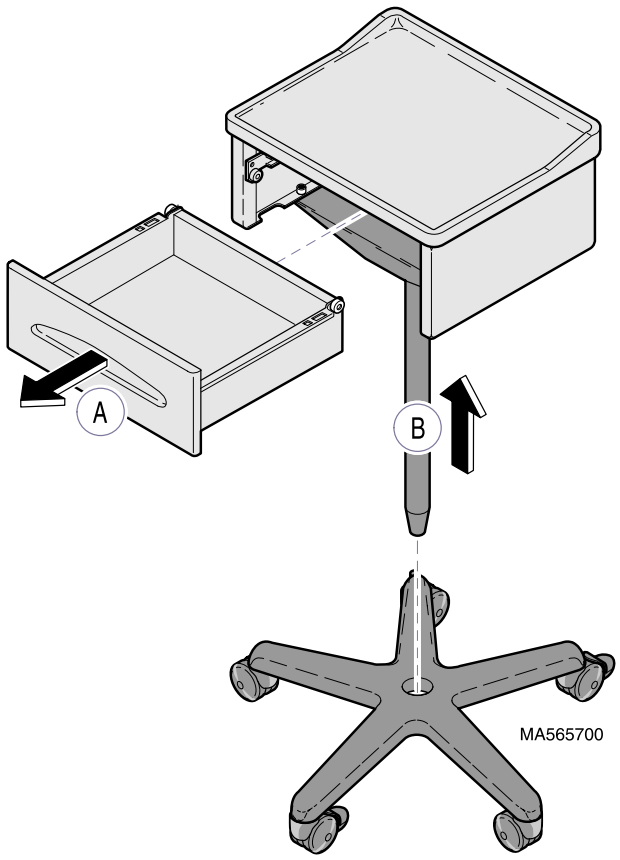

NOTE

Before working on ECG Cart remove all contents from top of cart and from drawer.

A. Remove drawer.

B. Separate caster base from pedestal by pulling upward.

NOTE

Lay unit on its side on a soft surface (to prevent scratching) for easier access when installing holder.

© Midmark Corporation - 2000

INSTALLATION

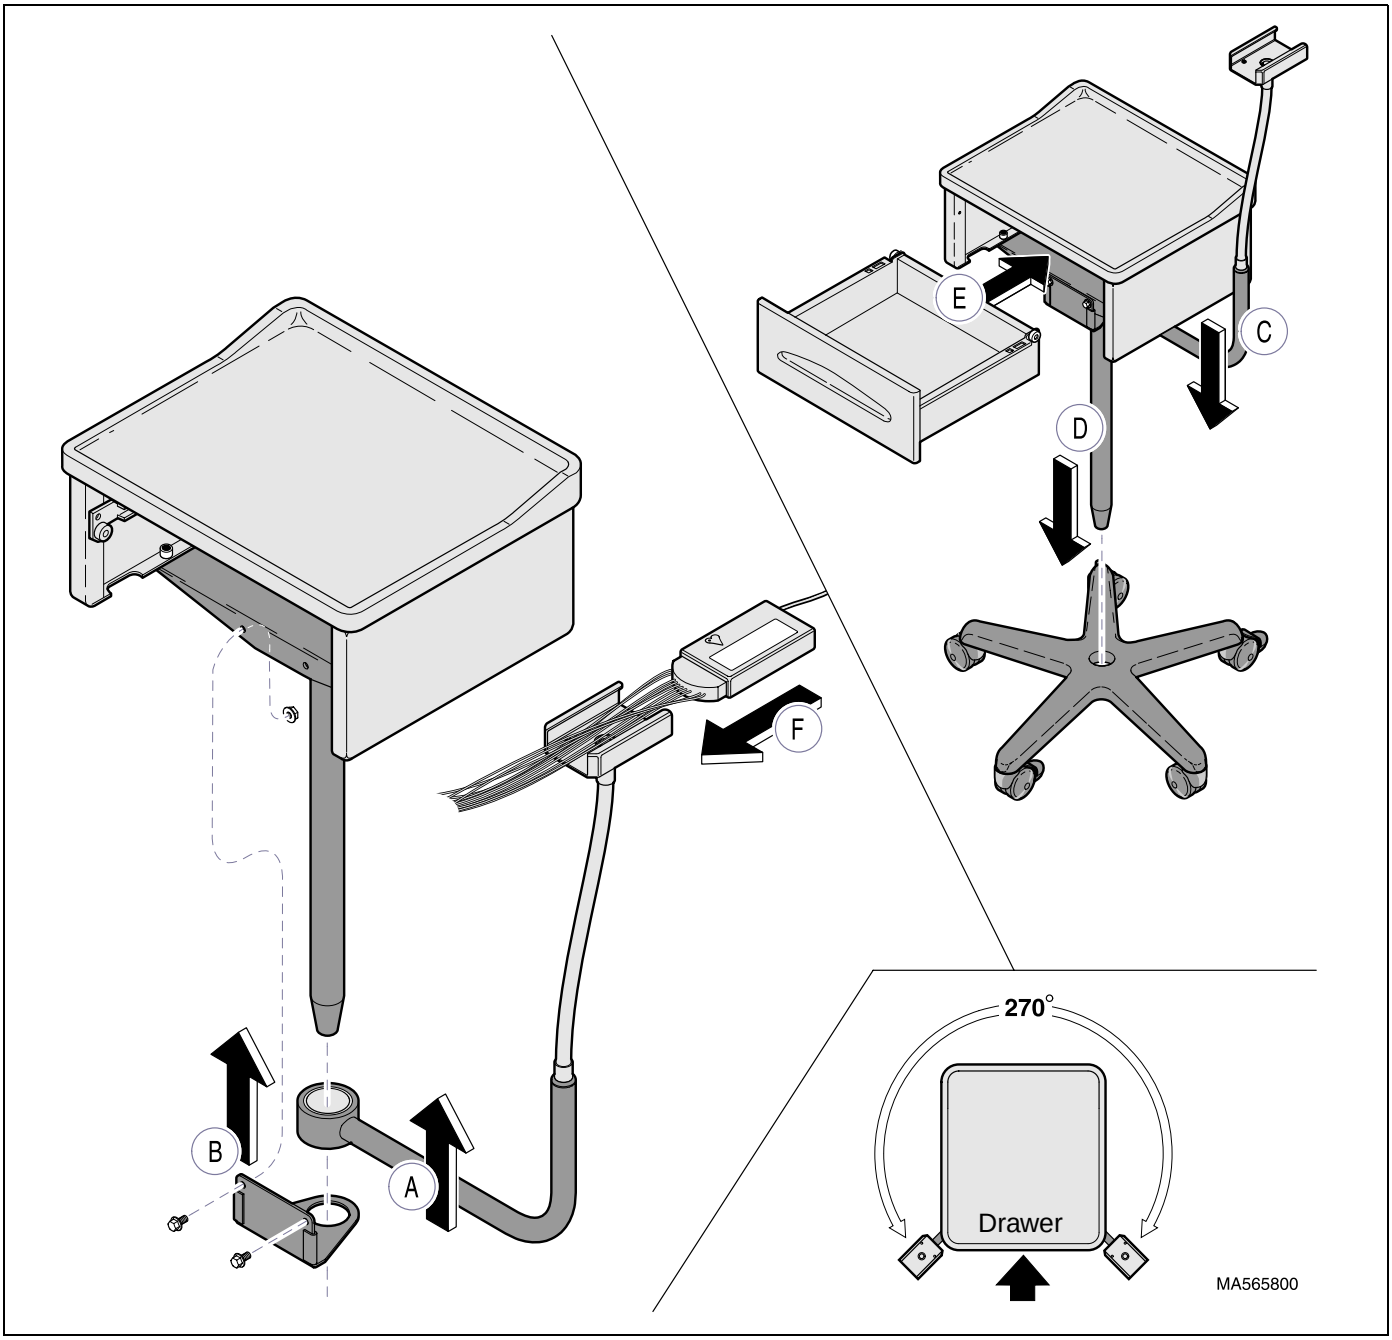

A. Position tube support / flex arm assembly onto cart post and slide to cabinet end .

B. With L-bracket positioned as shown, slide bracket onto cart post, align mounting holes of bracket with mounting holes of cabinet base. Secure with two 1/4"-20 x 1/2" bolts and nuts.

C. Position tube support / flex arm to rest on L-bracket.

D. Insert pedestal into caster base, pressing firmly downward.

E. Install drawer and check operation.

NOTE

The IQmark™ Flexible Rotating Mount should swing freely 270° from drawer corner to drawer corner.

F. Insert the IQmark™ ECG module into the holder as shown to lock it into position.

EQUIPMENT ALERT

Failure to properly install ECG module in holder could result in damage to equipment.

MIDMARK®
Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

© Midmark Corporation - 2000